




Technical data sheet

LLG-Screw Neck Vials N 9

Art.-Nr.: 4.008 250

NOTE: 1: * TO WITHSTAND A FORCE OF 10 NEWTONS
MIN. AT 25 / 27 FROM NECK
2: INSERT SHOULD BE FLUSH WITH THE PARENT
VIAL AT THE OPEN END ± 0.25

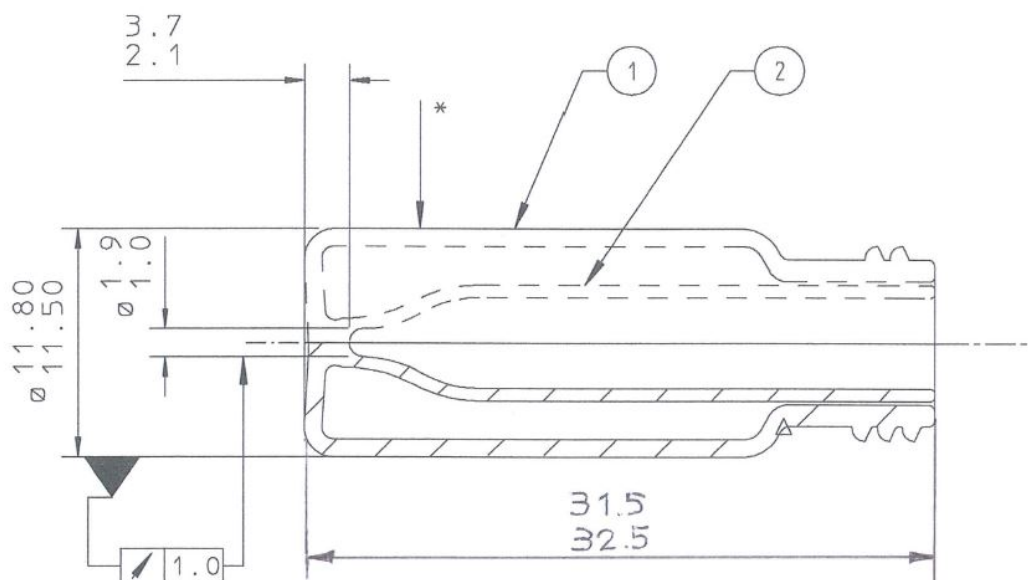

This document was sent online and is valid without signature